


Operative hysteroscopy
without capital cost
or complexity



LiNA OperåScope™

The complete single-use system for see
and treat hysteroscopy in the office.

LiNA
®

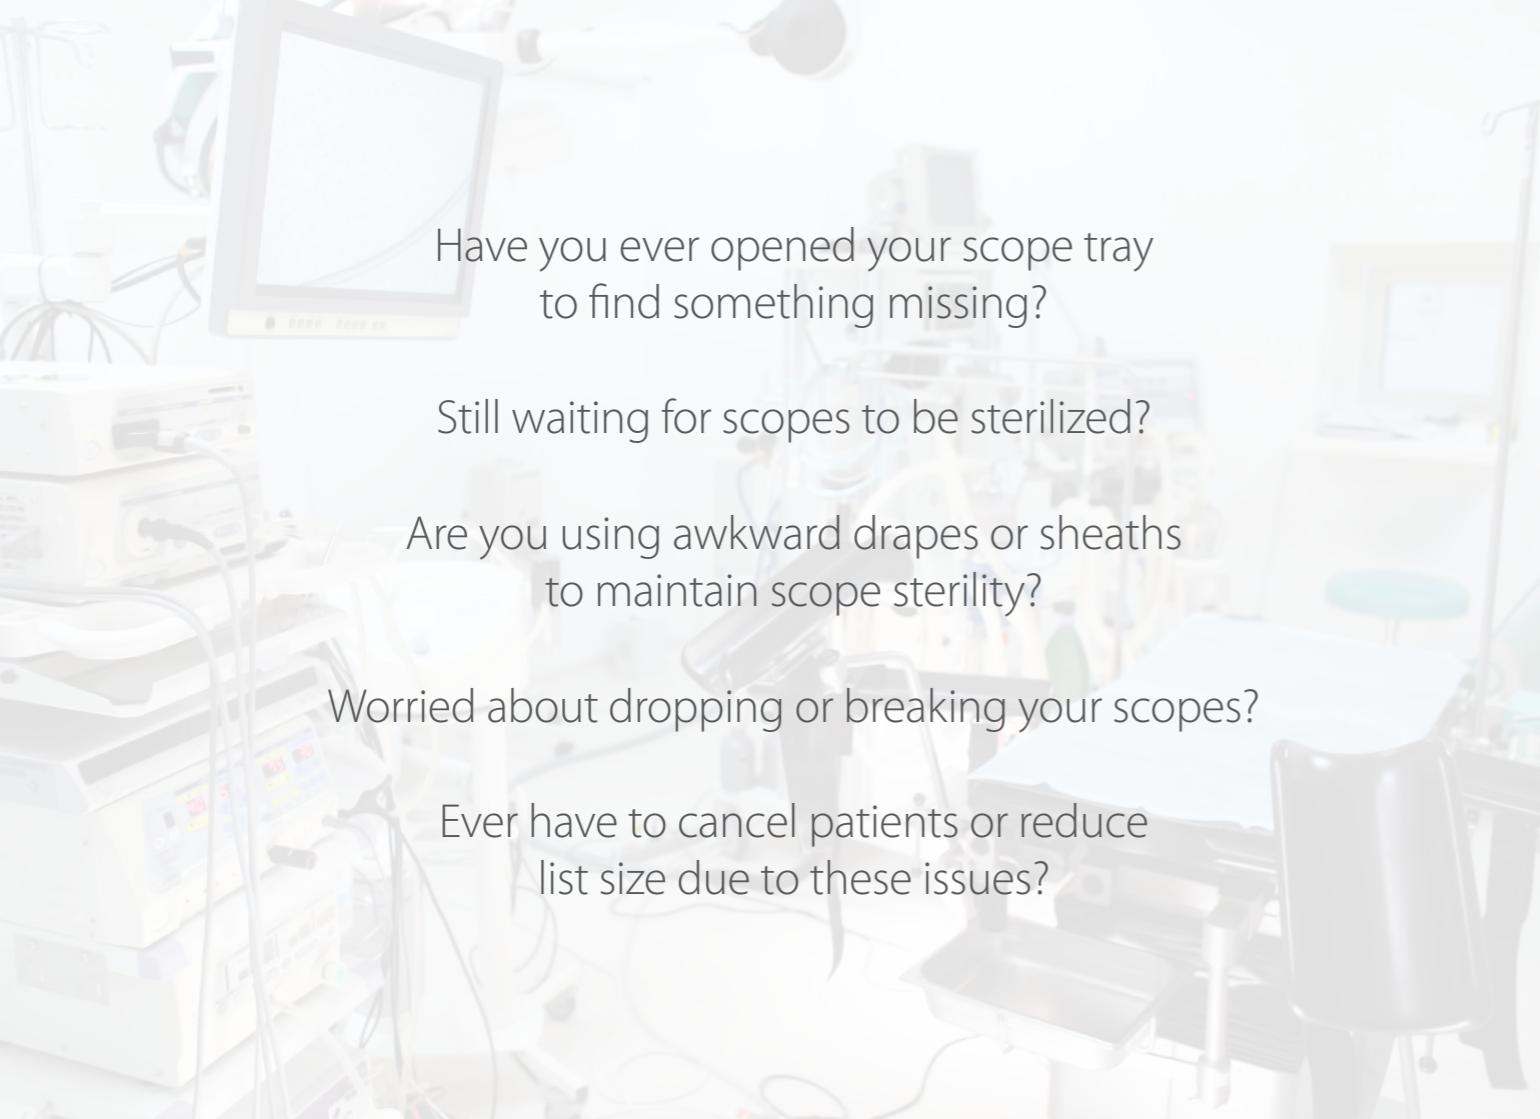

Have you ever opened your scope tray
to find something missing?

Still waiting for scopes to be sterilized?

Are you using awkward drapes or sheaths
to maintain scope sterility?

Worried about dropping or breaking your scopes?

Ever have to cancel patients or reduce
list size due to these issues?

Traditional hysteroscopy
can be complicated...

The cost and complexity of traditional equipment can make it difficult to incorporate hysteroscopy into your practice. You need staff, sterilization chemicals, and supplies... lots of supplies if you want to support multiple rooms and multiple patients in a day.




Turn every exam room
into a hysteroscopy
procedure room.



LiNA OperåScope™

The LiNA OperåScope™ was designed specifically with the office setting in mind. The convenient single-use design is ready for use out of the box, allowing you to diagnose and treat patients without the constraints of traditional hysteroscopy.


Curved tip to match her anatomy.
Ergonomic handle to match yours.

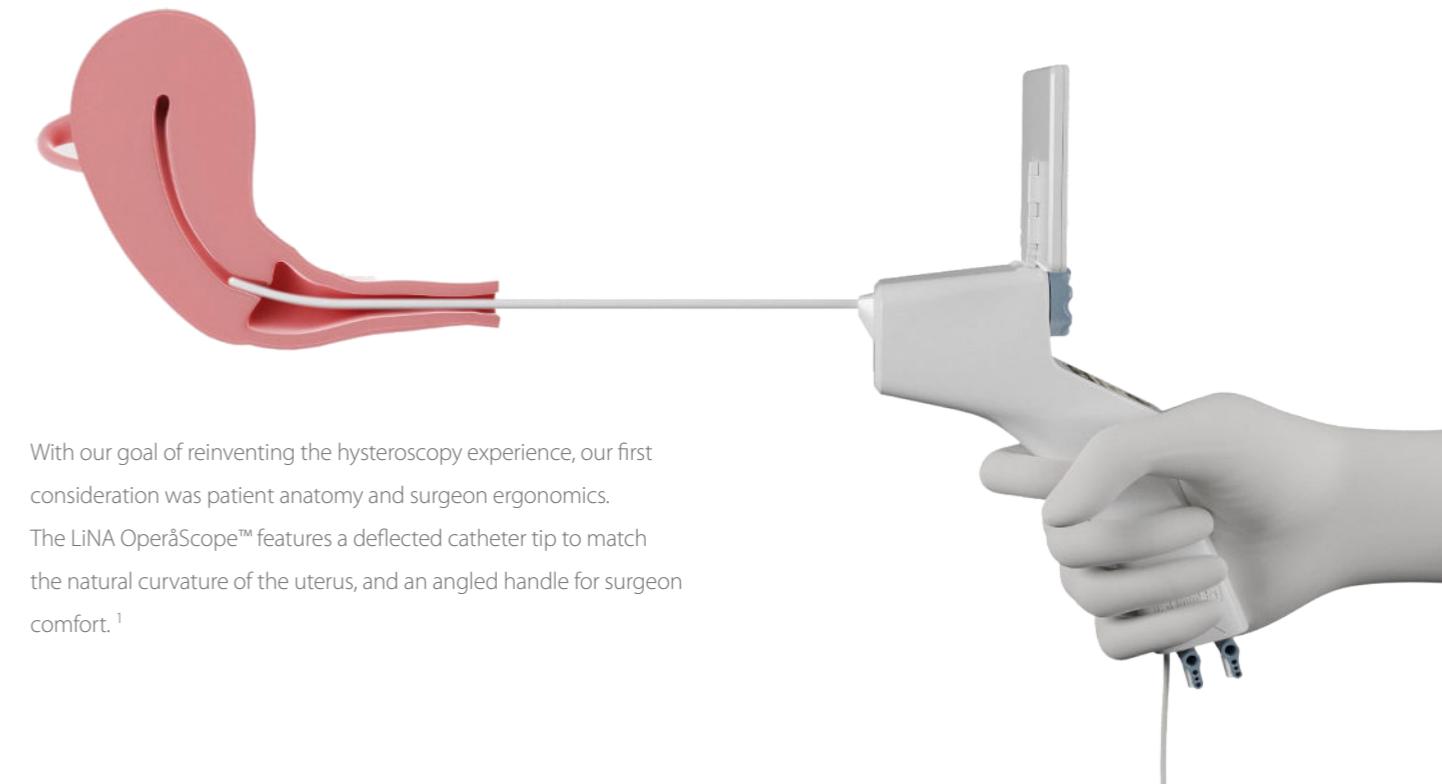

With our goal of reinventing the hysteroscopy experience, our first consideration was patient anatomy and surgeon ergonomics. The LiNA OperåScope™ features a deflected catheter tip to match the natural curvature of the uterus, and an angled handle for surgeon comfort.¹

The steerability and control you've been looking for.

Our rigid catheter and 360° steerable tip allows for precise control and maneuverability to navigate your patient's unique anatomy.

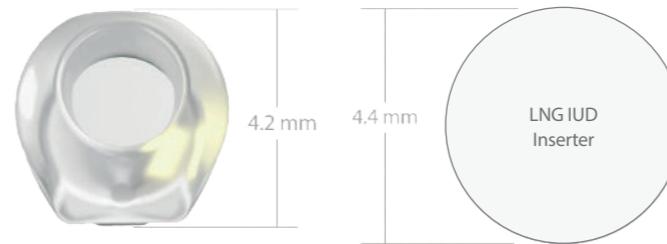

Slim catheter for less dilation and anesthesia.

State of the art micro camera technology has allowed us to create a catheter tip that's smaller than an LNG IUD inserter for improved patient tolerability.^{2,3}



Effective distention and clear visualization.

LiNA OperâScope™ features dedicated in-flow and out-flow channels with individual stop-cocks for optimal fluid management.



LiNA Tubing and Drape Kit.

We offer a convenient hysteroscopy tubing and drape kit to address your fluid management needs. Our kit includes:

Full under buttocks drape with graduation markings and drainage port.

Inflow tubing with luer lock connector and spike connector for use with saline bag.


Outflow tubing with luer lock connector and female suction cannister connector.

Drainage collection bag.



LiNA Single-Use Instrumentation.

LiNA OperåScope™ features a 5.5 french operative channel for therapeutic use. Our affordable selection of single-use instrumentation enables see and treat hysteroscopy without the constraints of traditional reusable instruments.

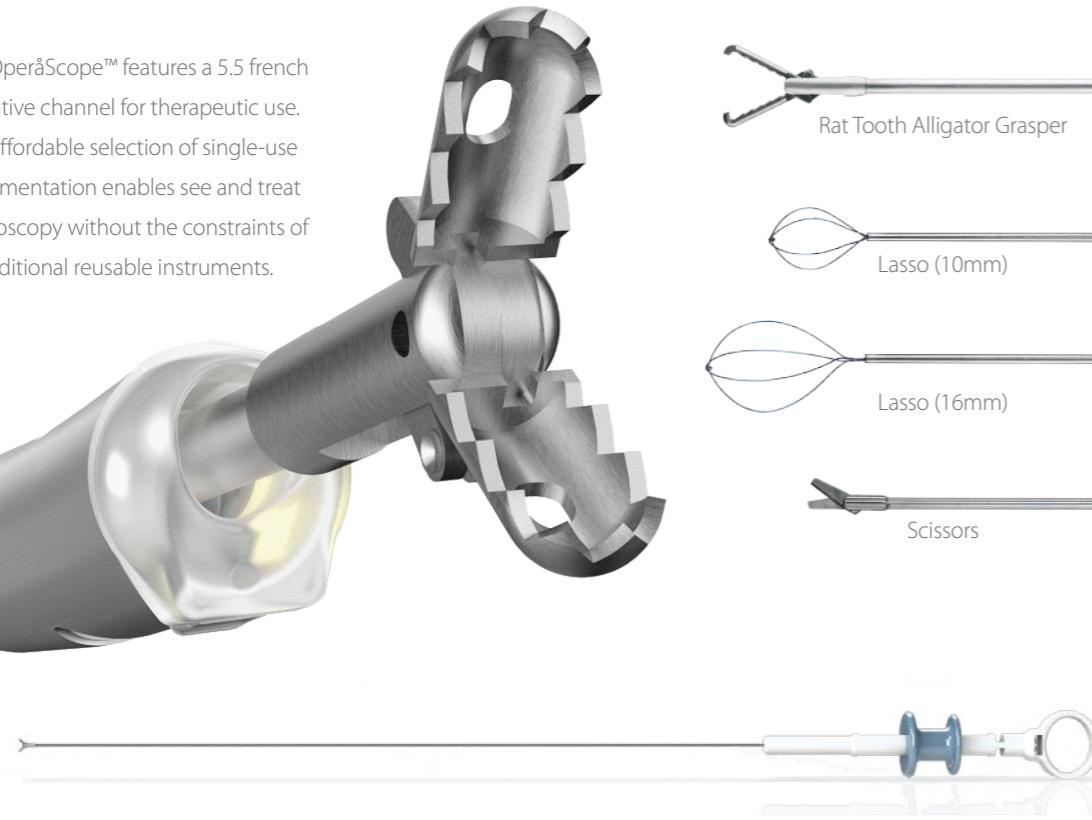

Recording and Connectivity.

The LiNA OperåScope™ offers multiple options to match your office setup and recording needs. You have the on board LCD viewing, connection to an external monitor of your choice via standard HDMI cable, video recording/ image capture via HDMI connection to the LiNA OperåScope™ Recording Module with USB drive and video recording/image capture and external monitor connectivity through the LiNA OperåScope™ Recording Module.



Ordering information

Product Code	Description	UOM
OP-201-6-I	LiNA OperaScope™ with HDMI cable & LCD	Box of 6ea
OP-FCP-6-I	LiNA OperaScope™ Biopsy Forceps, Alligator Biopsy Forceps for hysteroscopy. Minimum channel diameter: Ø1.87 mm	Box of 6ea
OP-GRA-6-I	LiNA OperaScope™ Rat Tooth Alligator Grasper, Rat Tooth Alligator Grasper for hysteroscopy. Minimum channel diameter: Ø1.87 mm	Box of 6ea
OP-LAS10-3-I	LiNA OperaScope™ Lasso 10mm Basket, Hysteroscopic Polyp Basket: Ø10 mm. Minimum channel diameter: Ø1.87 mm	Box of 3ea
OP-LAS16-3-I	LiNA OperaScope™ Lasso 16mm Basket, Hysteroscopic Polyp Basket: Ø16 mm. Minimum channel diameter: Ø1.87 mm	Box of 3ea
OP-RM-1-UK	LiNA OperaScope™ Recording Module – Socket Type G	Each
OP-RM-1-EU	LiNA OperaScope™ Recording Module – Socket Type C	Each
OP-RM-1-AUS	LiNA OperaScope™ Recording Module – Socket Type I	Each
OP-SCI-3-I	LiNA OperaScope™ Scissors, Scissors for hysteroscopy. Minimum channel diameter: Ø1.87 mm	Box of 3ea
OP-TDK-6-I	LiNA OperaScope™ Tubing & Drape Kit, Tubing & Drape for hysteroscopy	Box of 6ea

References:

1. Sallam, H. N., et al. "Ultrasound measurement of the uterocervical angle before embryo transfer: a prospective controlled study." *Human Reproduction* 17.7 (2002): 1767-1772.
2. Gemzell-Danielsson, Kristina, et al. "Overcoming barriers to levonorgestrel-releasing intrauterine system placement: an evaluation of placement of LNG-IUS 8 using the modified Evolnserter® in a majority nulliparous population." *Contraception* 96.6 (2017): 426-431.
3. Bednarek, Paula H., and Jeffrey T. Jensen. "Safety, efficacy and patient acceptability of the contraceptive and non-contraceptive uses of the LNG-IUS." *International journal of women's health* 1 (2009): 45.
4. Moustafa S, Rosen E, Goodman L. Patient and provider satisfaction with saline ultrasound versus office hysteroscopy for uterine cavity evaluation prior to in vitro fertilization: a randomized controlled trial. *J Assist Reprod Genet*. 2021 Mar;38(3):627-634.

Innovation in Gynecology



LiNA Medical AG - Platz 3 - 6039 Root D4 - Switzerland
Phone: +41 78 617 56 56, e-mail: info@lina-medical.com, www.linamed.com

EU REP

LiNA Medical Polska Sp. z o.o. - Rolna 8A - Sady - 62-080 Tarnowo Podgórne - Poland
Phone: +48 61 222 21 21, e-mail: info.poland@lina-medical.com, www.lina-medical.pl

Please refer to the Instruction for Use for complete instructions, contraindications, warnings and precautions.

EU MDR 2017/745 device class for REF:

- OP-201-6-I, OP-TDK-6-I: class IIa
- OP-SCI-3-I, OP-GRA-6-I, OP-LAS10-3-I, OP-LAS16-3-I, OP-FCP-6-I: class I
- OP-RM-1-EU, OP-RM-1-UK, OP-RM-1-AUS: class I

Name and number of the Notified Body: TUV Nord Polska Sp. z o.o. # 2274.

*EN ISO 13485:2016
Quality Management System*

LiNA OperaScope Physician Brochure 2025-10 BV0239D en

©2025 LiNA Medical AG. All rights reserved.

LiNA is a registered trademark of LiNA Medical in EU, US and CN.

